


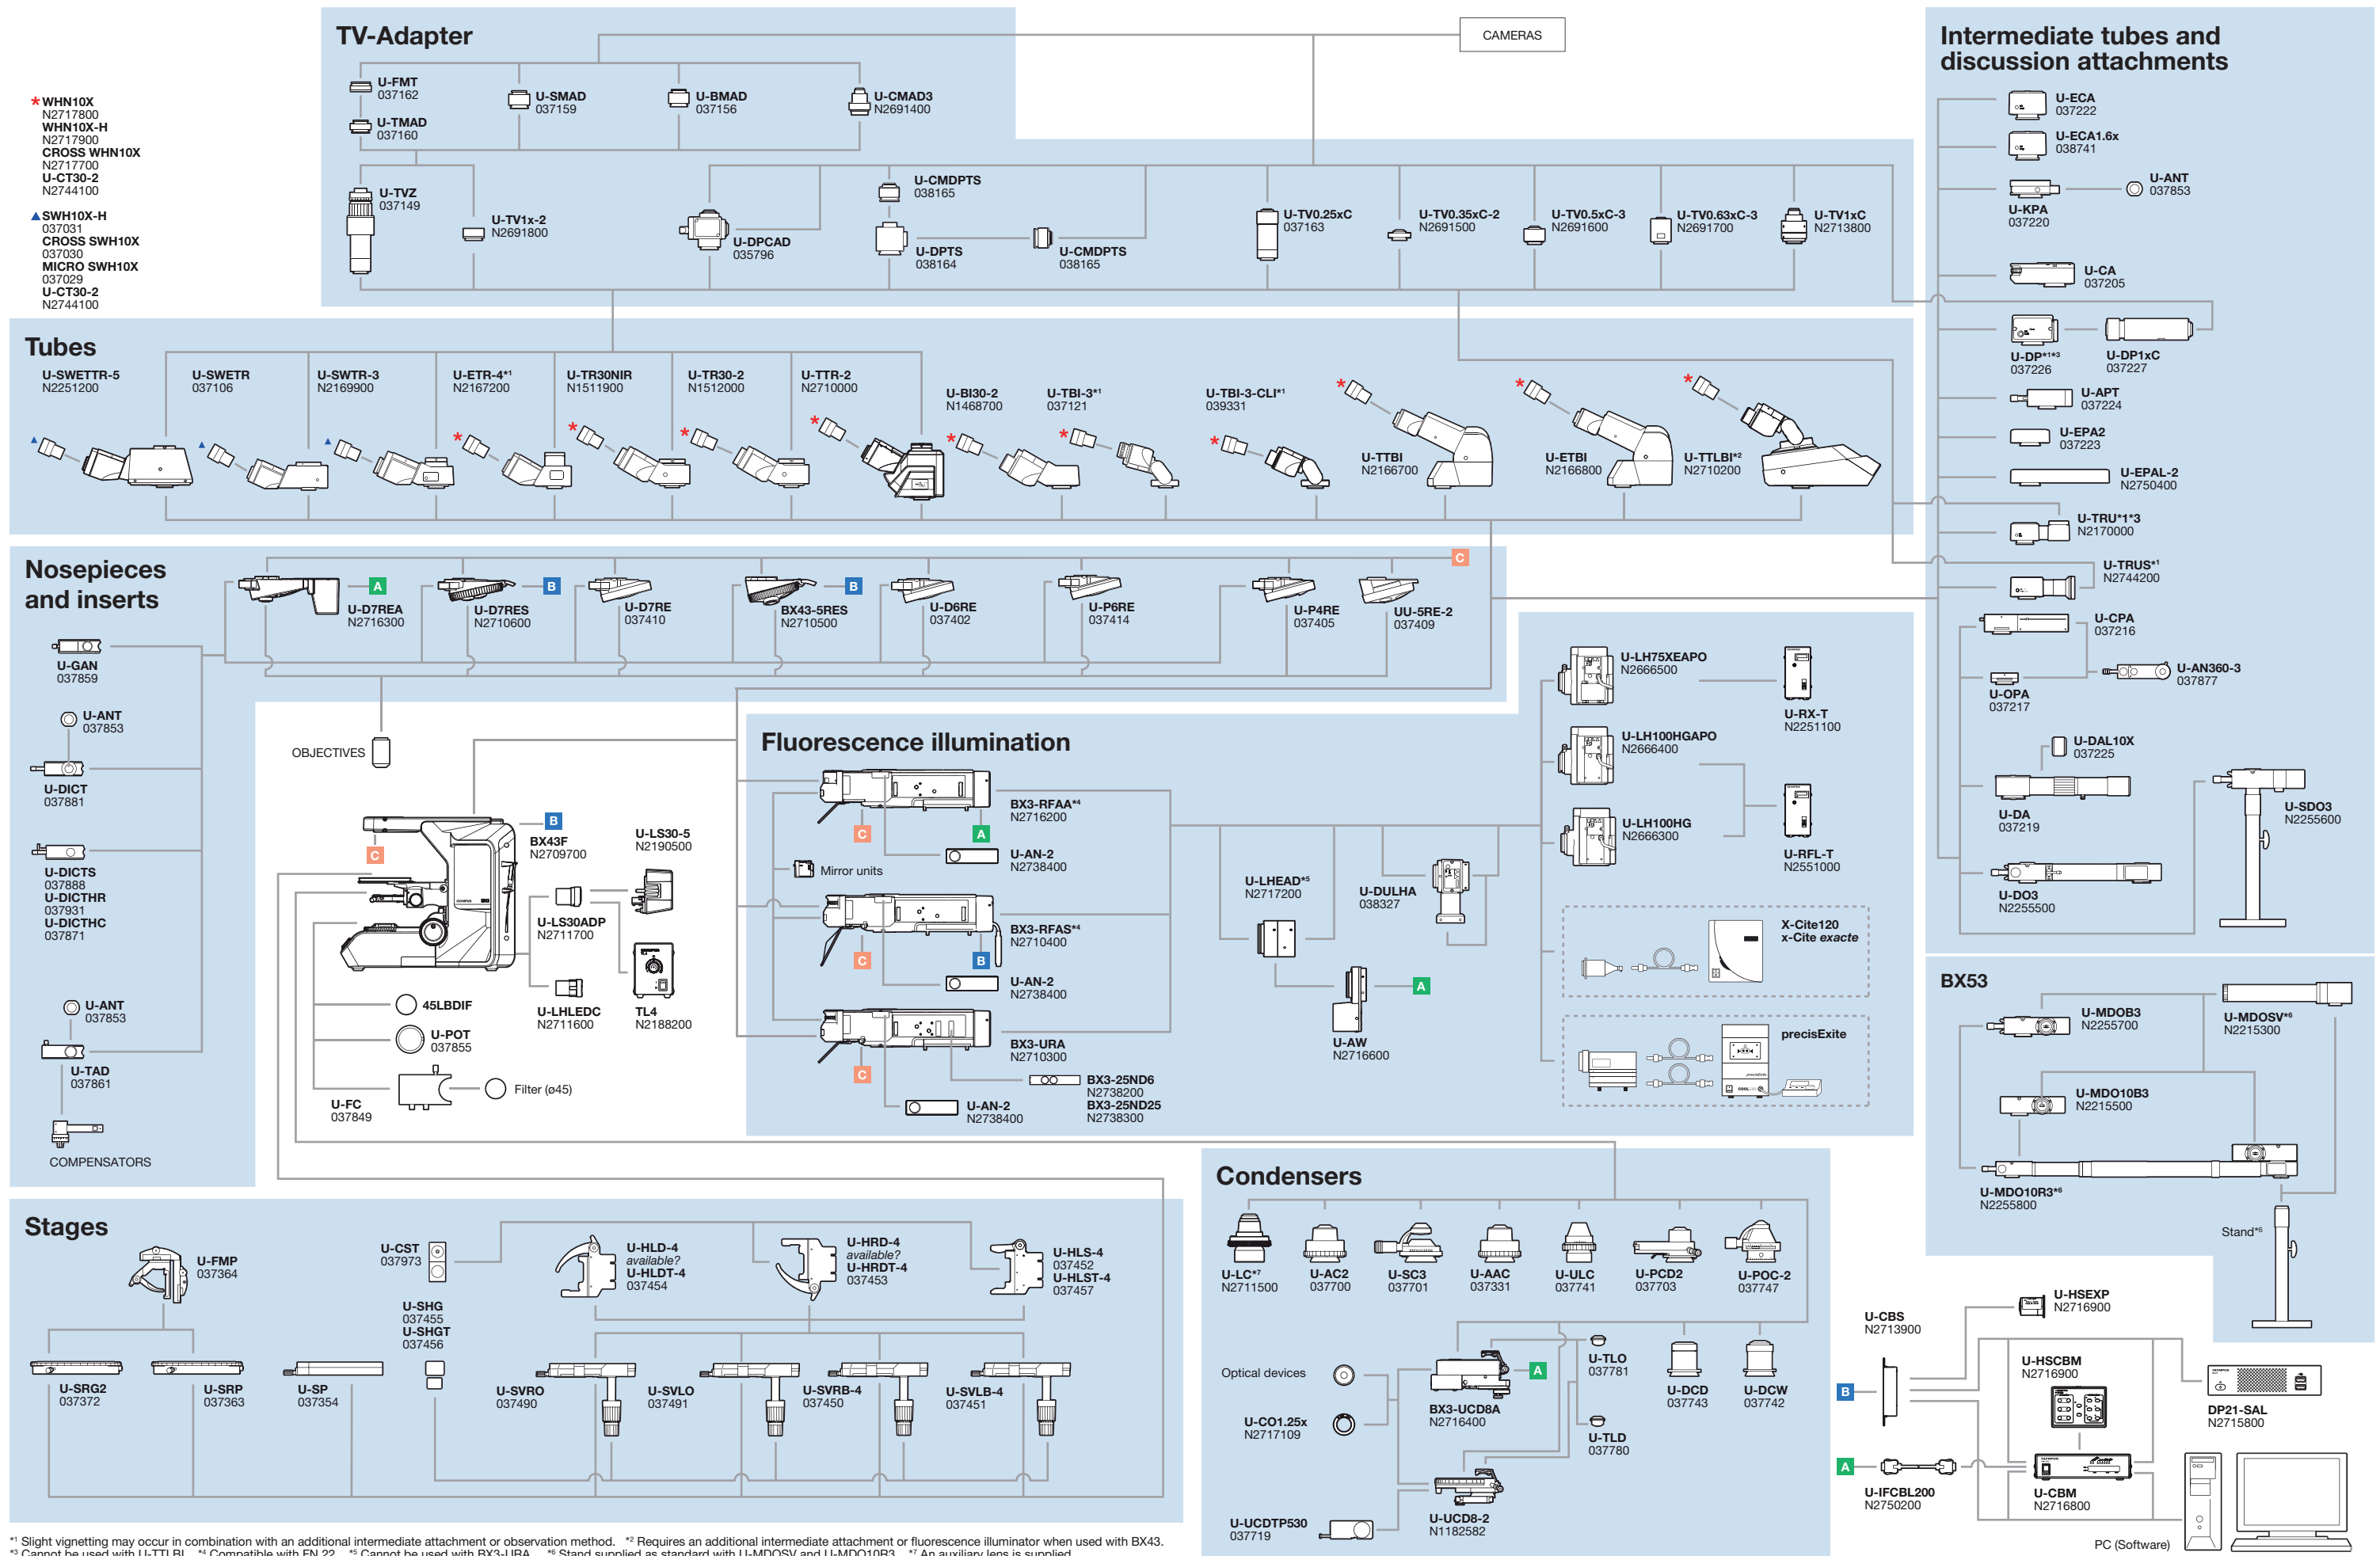

*1 Slight vignetting may occur in combination with an additional intermediate attachment or observation method. *2 Requires an additional intermediate attachment or fluorescence illuminator when used with BX43. *3 Cannot be used with U-TTLBI. *4 Compatible with FN 22. *5 Cannot be used with BX3-URA. *6 Stand supplied as standard with U-MDOSV and U-MDO10R3. *7 An auxiliary lens is supplied.